


Intended use :

This product is designed for use under recommendations from your health care professional or sleep therapist. This product is used on adult patients (weight above 30kg) whom CPAP or bi-level therapy has been prescribed. The product is re-usable for single patient in medical institutions, home care and sleep treatment center.

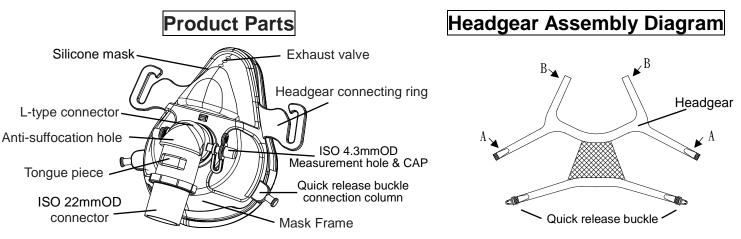

Instructions for use :

- Inspect the packaging and product appearance before using. Please do not use if there are any worn or damaged parts.
- Take out the mask set and L-type connector from the box and snap the L-type connector into the mask.
- See headgear assembly diagram, hook headgear point A to the mask frame connecting rings on both sides, and then bond the two B points.
- > Hold the mask over nose and mouth, and then position the headgear.
- > Fast release buckle to the mask frame Quick release buckle connection column.
- > Adjust the head straps and the hook and loop of the mask comfortably.
- > L-type connector side ISO 4.3mmOD hole for measurement monitoring use.
- > After wearing, connect the ventilation tube connector to the ISO 22mm OD for use.
- > Quick release buckle on both sides can be easily removed, also be connected easily.


♦ Cleaning :

- \diamond This product is reusable for single patient.
- ♦ Follow the procedures for cleaning/sterilization in medical institutions.
- ♦ Wash the headgear with warm water and neutral detergent or soap. After rinse, air-dry the strap and keep away from direct sunlight or the dryer.
- ♦ Mask and L-type connector can be disconnected for cleaning.
- \diamond Wash with warm water and neutral detergent or soap.
- \diamond After rinse, dry in a cool place. Do not put it in the dryer.
- The uncovered can be autoclaved 25 times with the 15minute*121°C high temperature steam (pressure) sterilization method.

- \triangle Multiple patients reuse will result in cross-infection of disease.
- △ Prohibit the use of if the patient has the following symptoms: vomiting, facial trauma burns, impaired myocardial function, Gastroesophageal Reflux Disease, abnormal cough reflex, unconsciousness.
- \bigtriangleup To be worn by professional medical staff guidance.
- \triangle Do not cover or block anti-asphyxiation holes and breathing valve.
- \triangle Do not connect worn breathing apparatus has not been started before operation.
- \triangle If you feel unwell, STOP using it immediately and seek medical advice immediately.
- \bigtriangleup Do not use alcohol \backsim bleach or solvents containing chlorine and other components to clean the mask set.
- \bigtriangleup Do not put the mask set and headgear in the place of the sun exposure or high temperature preservation.
- \bigtriangleup Do not dismantling the silicone mask and, this action will mask a small loss of functionality, and reduce product life.
- \triangle Occur in a leak, slight tightening of the headgear, no improvement in the condition of leakage and then gently tighten the headgear, do not force too much cause discomfort.
- \triangle Dispose of it according to the local medical waste disposal regulations.

• Specifications and materials :

- Double Layer Mask size : S / M / L.
- L-type connector : 22mmOD meet ISO 5356-1.
- Headgear : General.

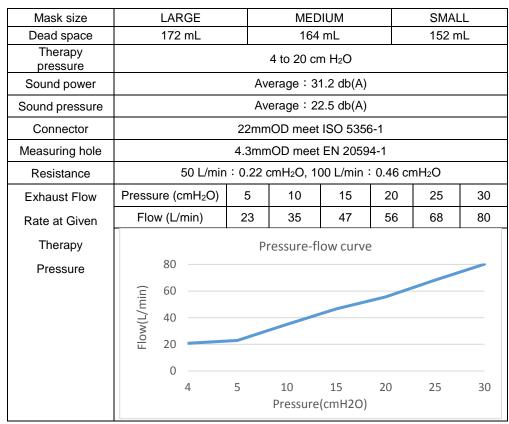



IFU-1631 REV 01

EC REP

Obelis s.a. Boulevard Général Wahis 53 1030 Brussels, BELGIUM Tel : +(32) 2.732.59.54 Fax : +(32)2.732.60.03 E-Mail : mail@obelis.net



Manufacturer : DA CHUNG MEDICAL CO., LTD. Address : No. 600, Sec. 1, Dong Shan Rd., Dong Shan Township, Yilan County, Taiwan. TEL: +886 3 959 4777 Website : http://www.dc-med.com.tw